PWLS-ULTRA: An Efficient Clustering and Learning-Based Approach for Low-Dose 3D CT Image Reconstruction

Xuehang Zheng, Saiprasad Ravishankar, *Member, IEEE*, Yong Long*, and Jeffrey A. Fessler, *Fellow, IEEE*

arXiv:1703.09165v1 [stat.ML] 27 Mar 2017

***Abstract*—The development of computed tomography (CT) image reconstruction methods that significantly reduce patient radiation exposure while maintaining high image quality is an important area of research in low-dose CT (LDCT) imaging. We propose a new penalized weighted least squares (PWLS) reconstruction method that exploits regularization based on an efficient Union of Learned TRAnsforms (PWLS-ULTRA). The union of square transforms is pre-learned from numerous image patches extracted from a dataset of CT images or volumes. The proposed PWLS-based cost function is optimized by alternating between an image update step, and a sparse coding and clustering step. The CT image update step is accelerated by a relaxed linearized augmented Lagrangian method with ordered-subsets that reduces the number of forward and backward projections. Simulations with 2D and 3D axial CT scans of the XCAT phantom and 3D helical chest scans show that for low-dose levels, the proposed method significantly improves the quality of reconstructed images compared to PWLS reconstruction with a nonadaptive edge-preserving regularizer (PWLS-EP). PWLS with regularization based on a union of learned transforms leads to better image reconstructions than using a single learned square transform or a learned overcomplete synthesis dictionary. We also incorporate patch-based weights in PWLS-ULTRA that enhance image quality and help improve image resolution uniformity.**

***Index Terms*—Low-dose CT, statistical image reconstruction, sparse representations, sparsifying transform learning, dictionary learning, machine learning**

I. Introduction

There is a growing interest in techniques for computed tomography (CT) image reconstruction that significantly reduce patient radiation exposure while maintaining high image quality. Dictionary learning based techniques have been proposed for low-dose CT (LDCT) imaging, but often involve expensive computation. This paper proposes a new penalized weighted least aquares (PWLS) reconstruction approach that exploits regularization based on an efficient Union of Learned TRAnsforms (PWLS-ULTRA). In the following, we briefly review recent methods for LDCT image reconstruction and summarize the contributions of this work.

This work was supported in part by the SJTU-UM Collaborative Research Program, NSFC (61501292), Shanghai Pujiang Talent Program (15PJ1403900), NIH grant U01 EB018753, ONR grant N00014-15-1-2141, DARPA Young Faculty Award D14AP00086, and ARO MURI grants W911NF-11-1-0391 and 2015-05174-05. *Asterisk indicates the corresponding author.*

X. Zheng and Y. Long are with the University of Michigan - Shanghai Jiao Tong University Joint Institute, Shanghai Jiao Tong University, Shanghai 200240, China (email: zhxhang@sjtu.edu.cn, yong.long@sjtu.edu.cn)

S. Ravishankar and J. A. Fessler are with the Department of Electrical Engineering and Computer Science, University of Michigan, Ann Arbor, MI, 48109 USA (email: ravisha@umich.edu, fessler@umich.edu)

A. Background

Various methods have been proposed for image reconstruction in LDCT imaging. When radiation dose is reduced, analytical filtered back-projection (FBP) image reconstruction methods (e.g., the Feldkamp-Davis-Kress or FDK method [1]) typically provide unacceptable image quality. For example, streak artifacts increase severely as radiation dose is reduced [2]. Model-based image reconstruction (MBIR) methods, aka statistical image reconstruction (SIR) methods, can provide high-quality reconstructions from low-dose scans [3], [4]. These methods iteratively find the image based on the system (physical) model, the measurement statistical model, and (assumed) prior information about the unknown object. A typical MBIR method for CT uses a penalized weighted-least squares (PWLS) cost function with a statistically weighted quadratic data-fidelity term and a penalty term (regularizer) modeling prior knowledge of the underlying unknown object [5]–[7]. Current commercially available LDCT image reconstruction methods, including MBIR with edge-preserving (or total variation) regularization and FBP followed by post-processing denoising steps, use very simple prior information. Adopting better image priors in MBIR could substantially improve image reconstruction quality for LDCT scans.

Extracting prior information from big datasets of regular dose CT images has great potential to enable MBIR methods to produce significantly improved reconstructions from LDCT measurements. For example, images are often sparse in certain transform domains (such as wavelets, discrete cosine transform, and discrete gradient) or dictionaries. The synthesis dictionary model approximates a signal by a linear combination of a few columns or atoms of a pre-specified dictionary [8]. The choice of the synthesis dictionary is critical for the success of sparse representation modeling and other applications [9]. The data-driven adaptation of dictionaries, or dictionary learning [10]–[14] yields dictionaries with better sparsifying capability for specific classes of signals than analytic dictionaries based on mathematical models. Such learned dictionaries have been widely exploited in various applications in recent years, including super-resolution imaging, image or video denoising, classification, and medical image reconstruction [15]–[21]. Some recent works also studied parametrized models such as adaptive tight frames [22], multivariate Gaussian mixture distributions [23], and shape dictionaries [24].

Recently, Xu *et al.* [25] applied dictionary learning to 2D LDCT image reconstruction by proposing a PWLS approach

with an overcomplete synthesis dictionary-based regularizer. Their method uses either a global dictionary trained from 2D image patches extracted from a normal-dose FBP image, or an adaptive dictionary jointly estimated with the low-dose image. The trained global dictionary worked better than the adaptively estimated dictionary for highly limited (e.g., with very few views, or ultra-low dose) data. Several works proposed 3D CT reconstruction by learning either a 3D dictionary from 3D image patches, or learning three 2D dictionaries (dubbed 2.5D) from image patches extracted from slices along the x-y, y-z, and x-z directions, respectively [26], [27].

Dictionary learning methods typically alternate between estimating the sparse coefficients of signals or image patches (*sparse coding step*) and updating the dictionary (*dictionary update step*). The sparse coding step in both synthesis dictionary learning [12], [15] and analysis dictionary learning [28] is NP-Hard (Non-deterministic Polynomial-time hard) in general, and algorithms such as K-SVD [12], [15] involve relatively expensive computations for sparse coding. A recent generalized analysis dictionary learning approach called sparsifying transform learning [29], [30] more efficiently learns a transform model for signals. The transform model assumes that a signal $\mathbf{x} \in \mathbb{R}^n$ is approximately sparsifiable using a transform $\mathbf{\Omega} \in \mathbb{R}^{m \times n}$, i.e., $\mathbf{\Omega x} = \mathbf{z} + \mathbf{e}$ where $\mathbf{z} \in \mathbb{R}^m$ is sparse in some sense, and $\mathbf{e} \in \mathbb{R}^m$ denotes modeling error in the transform domain. Transform learning methods typically alternate between sparse approximation of signals in the transform domain (*sparse coding step*) and updating the transform operator (*transform update step*). In contrast to dictionary learning methods, the sparse coding step in transform learning involves simple thresholding [29], [30]. Transform learning methods have been recently demonstrated to work well in applications [31]–[34]. Pfister and Bresler [35]–[37] showed the promise of PWLS reconstruction with adaptive square transform-based regularization, wherein they jointly estimated the square transform (ST) and the image. Pre-training a (global) transform from a large dataset would save computations during CT image reconstruction, and may also be well-suited for highly limited data (evidenced earlier for dictionary learning in [25]).

Wen *et al.* recently extended the single ST learning method to learning a union of square transforms model, also referred to as an overcomplete transform with block cosparsity (OCTOBOS) [38]. This transform learning approach jointly adapts a collection (or union) of K square transforms and clusters the signals or image patches into K groups. Each (learned) group of signals is well-matched to a corresponding transform in the collection. Such a learned union of transforms outperforms the ST model in applications such as image denoising [38].

B. Contributions

Incorporating the efficient square transform (ST) model, we propose a new PWLS approach for LDCT reconstruction that exploits regularization based on a pre-learned square transform (PWLS-ST). We also extend this approach to a more general PWLS scheme involving a union of learned transforms (PWLS-ULTRA). The transform models are pre-learned from numerous patches extracted from a dataset of CT images or volumes. We also incorporate patch-based weights in the proposed regularizer to help improve resolution or noise uniformity. We propose an efficient iterative algorithm that alternates between a *sparse coding and clustering step* that uses closed-form solutions, and an iterative *image update step*. There are several iterative algorithms that could be used for the image update step such as the preconditioned conjugate gradient (PCG) method [39], the separable quadratic surrogate method with ordered-subsets based acceleration (OS-SQS) [40], iterative coordinate descent (ICD) [41], splitting-based algorithms [42], and the optimal gradient method (OGM) [43]. We chose the relaxed linearized augmented Lagrangian method with ordered-subsets (relaxed OS-LALM) [44] for the image update step.

The proposed PWLS-ULTRA approach clusters the voxels into different groups. These groups often capture features such as bones, specific soft tissues, edges, etc. Experiments with 2D and 3D axial CT scans of the XCAT phantom and 3D helical chest scans show that for low-dose levels, the proposed methods significantly improve the quality of reconstructed images compared to conventional reconstruction methods such as filtered back-projection or PWLS reconstruction with a nonadaptive edge-preserving regularizer (PWLS-EP). Using a union of learned transforms provides better images than using a single learned square transform or a learned overcomplete synthesis dictionary.

We presented a brief study of PWLS-ST for low-dose fan-beam (2D) CT image reconstruction in [45]. This paper investigates the more general PWLS-ULTRA framework, and presents experimental results illustrating the properties of the PWLS-ST and PWLS-ULTRA algorithms and demonstrating their performance for low-dose fan-beam, cone-beam (3D) and helical (3D) CT.

C. Organization

Section II describes the formulations for pre-learning a square transform or a union of transforms, and the formulations for PWLS reconstruction with regularization based on learned sparsifying transforms. Section III derives efficient optimization algorithms for the proposed problems. Section IV presents experimental results illustrating properties of the proposed algorithms and demonstrating their promising performance for LDCT reconstruction compared to numerous recent methods. Section V presents our conclusions and mentions areas of future work.

II. Problem Formulations for Transform Learning and Image Reconstruction

A. PWLS-ST Formulation for LDCT Reconstruction

Given N' vectorized image patches (2D or 3D) extracted from a dataset of regular dose CT images or volumes, we learn a square transform $\mathbf{\Omega} \in \mathbb{R}^{l \times l}$ by solving the following (training) optimization problem:

$$\min_{\mathbf{\Omega}, \mathbf{Z}} \|\mathbf{\Omega X} - \mathbf{Z}\|_F^2 + \lambda Q(\mathbf{\Omega}) + \sum_{i=1}^{N'} \eta^2 \|\mathbf{Z}_i\|_0 \qquad \text{(P0)}$$

where l is the size of each patch, $\lambda = \lambda_0 \|\mathbf{X}\|_F^2$ ($\lambda_0 > 0$ is a constant) and $\eta > 0$ are scalar parameters, and $\{\mathbf{Z}_i\}_{i=1}^{N'}$

denote the sparse codes of the training signals (vectorized patches) $\{\mathbf{X}_i\}_{i=1}^{N'}$. Matrices $\mathbf{X} \in \mathbb{R}^{l \times N'}$ and $\mathbf{Z} \in \mathbb{R}^{l \times N'}$ have the training signals and sparse codes respectively, as their columns. The ℓ_0 "norm" counts the number of non-zeros in a vector. The term $\|\mathbf{\Omega X} - \mathbf{Z}\|_F^2$ is called the sparsification error and measures the deviation of the signals in the transform domain from their sparse approximations. Regularizer $Q(\mathbf{\Omega}) \triangleq \|\mathbf{\Omega}\|_F^2 - \log|\det \mathbf{\Omega}|$ prevents trivial solutions and controls the condition number of $\mathbf{\Omega}$ [30].

After a transform $\mathbf{\Omega}$ is learned, we reconstruct an (vectorized) image or volume $\mathbf{x} \in \mathbb{R}^{N_p}$ from noisy sinogram data $\mathbf{y} \in \mathbb{R}^{N_d}$ by solving the following optimization problem [45]:

$$\min_{\mathbf{x} \succeq \mathbf{0}} \frac{1}{2}\|\mathbf{y} - \mathbf{A}\mathbf{x}\|_{\mathbf{W}}^2 + \beta \mathsf{R}(\mathbf{x}) \tag{P1}$$

where $\mathbf{W} = \mathsf{diag}\{w_i\} \in \mathbb{R}^{N_d \times N_d}$ is the diagonal weighting matrix with elements being the estimated inverse variance of y_i [6], $\mathbf{A} \in \mathbb{R}^{N_d \times N_p}$ is the system matrix of a CT scan, the parameter $\beta > 0$ controls the noise and resolution trade-off, and the regularizer $\mathsf{R}(\mathbf{x})$ based on $\mathbf{\Omega}$ is defined as

$$\mathsf{R}(\mathbf{x}) \triangleq \min_{\{\mathbf{z}_j\}} \sum_{j=1}^{\tilde{N}} \left\{ \tau_j \|\mathbf{\Omega} \mathbf{P}_j \mathbf{x} - \mathbf{z}_j\|_2^2 + \gamma^2 \|\mathbf{z}_j\|_0 \right\} \tag{1}$$

where $\tilde{N}$ is the number of image patches, the operator $\mathbf{P}_j \in \mathbb{R}^{l \times N_p}$ extracts the jth patch of l voxels of $\mathbf{x}$ as $\mathbf{P}_j\mathbf{x}$, and vector $\mathbf{z}_j \in \mathbb{R}^l$ denotes the transform-sparse representation of $\mathbf{P}_j\mathbf{x}$. The regularizer includes a sparsification error term and a ℓ_0 "norm"-based sparsity penalty with weight γ^2 ($\gamma > 0$).

We also propose patch-based weights $\{\tau_j\}$ in (1) to encourage uniform spatial resolution or uniform noise in the reconstructed image [46] as follows:

$$\tau_j \triangleq \|\mathbf{P}_j \boldsymbol{\kappa}\|_1 / l \tag{2}$$

with $\boldsymbol{\kappa}$ (of same size as $\mathbf{x}$) whose elements κ_j are defined in terms of the entries of $\mathbf{A}$ (denoted a_{ij}) and $\mathbf{W}$ as $\kappa_j \triangleq \sqrt{\sum_{i=1}^{N_d} a_{ij} w_i / \sum_{i=1}^{N_d} a_{ij}}$ [47, eq(39)]. While the ℓ_1 norm, corresponding to the mean value of $\mathbf{P}_j\boldsymbol{\kappa}$, was used to define τ_j, we have observed that other alternative norms also work well in practice for LDCT reconstruction.

Fig. 1 shows example transforms (rows of $\mathbf{\Omega}$ are reshaped as $8 \times 8 \times 5$ patches and the first 8×8 slices of 256 such 3D patches are shown) learned from $8 \times 8 \times 5$ patches of an XCAT phantom [48] volume. The transform learned with $\eta = 150$ in (P0) has more oriented features whereas the transform learned with $\eta = 100$ shows more gradient (or finite-difference) type features. When these transforms were used to reconstruct a different test volume from low-dose cone-beam sinogram data, the transform with $\eta = 100$ provided a lower overall reconstruction error (RMSE) as the gradient-like features are good sparsifiers for the largely smooth parts of the image, but the transform with $\eta = 150$ provided a better reconstruction of edges and achieved a higher structural similarity (SSIM [49]) metric for the reconstruction due to the oriented (or edge like) features. This suggests that a single ST may not be rich enough to capture the diverse features, edges, and other properties of CT volumes. Therefore, next we extend the ST approach to a rich union of learned transforms scheme.

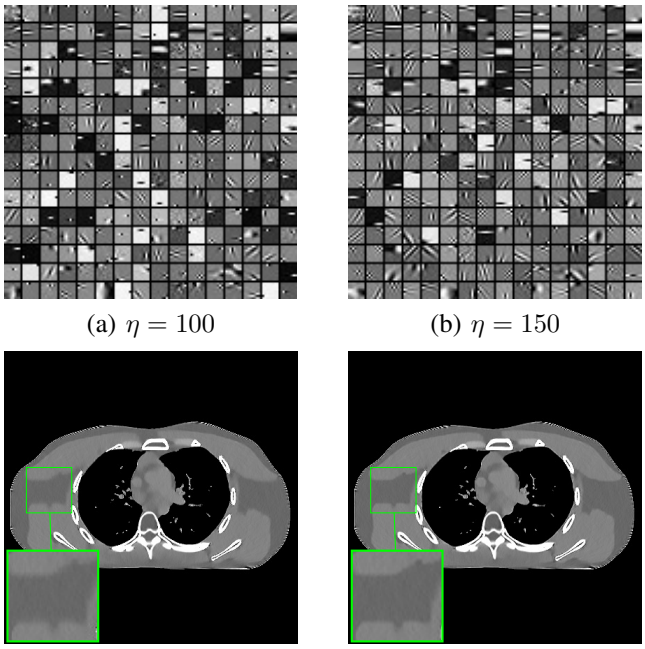

(a) $\eta = 100$ (b) $\eta = 150$ (c) (d)

Fig. 1. Behavior of PWLS-ST: Pre-learned $\mathbf{\Omega}$ with (a) $\eta = 100$ and (b) $\eta = 150$. The rows of the 320×320 matrix $\mathbf{\Omega}$ are reshaped into $8 \times 8 \times 5$ (3D) patches and the first 8×8 slices of 256 of these 3D patches are displayed for simplicity. (c) and (d) correspond to a slice (display window $[800, 1200]$ HU) of the 3D volumes reconstructed (root mean square error (RMSE) and structural similarity (SSIM) of 34.3 and 0.975, and 35.8 and 0.976, respectively for the volumes) from LDCT data using $\mathbf{\Omega}$ in (a) and (b), respectively.

B. Learning a Union of Sparsifying Transforms

Here, we learn a union of sparsifying transforms $\{\mathbf{\Omega}_k\}_{k=1}^K$ from N' (vectorized) patches by solving

$$\min_{\{\mathbf{\Omega}_k, \mathbf{Z}_i, C_k\}} \sum_{k=1}^{K} \sum_{i \in C_k} \left\{ \|\mathbf{\Omega}_k \mathbf{X}_i - \mathbf{Z}_i\|_2^2 + \eta^2 \|\mathbf{Z}_i\|_0 \right\} + \sum_{k=1}^{K} \lambda_k Q(\mathbf{\Omega}_k) \quad \text{s.t.} \quad \{C_k\} \in \mathcal{G}. \tag{P2}$$

This formulation groups the training signals $\{\mathbf{X}_i\}$ into K classes according to the transform they best match, and C_k denotes the set of indices of signals matched to the kth class. Set $\mathcal{G}$ denotes all possible partitionings of $\{1, 2, .., N'\}$ into K disjoint subsets. We use K regularizers $Q(\mathbf{\Omega}_k) \triangleq \|\mathbf{\Omega}_k\|_F^2 - \log|\det \mathbf{\Omega}_k|$, $1 \leq k \leq K$, to control the properties of the transforms. We set these regularizer weights as $\lambda_k = \lambda_0 \|\mathbf{X}_{C_k}\|_F^2$ [38], where $\lambda_0 > 0$ is a constant and $\mathbf{X}_{C_k}$ is a matrix whose columns are the training signals in the kth cluster. This choice of $\{\lambda_k\}$ together with $\eta = \eta_0 \|\mathbf{X}\|_F$ for $\eta_0 > 0$ allows the terms in (P2) to scale appropriately with the data. Problem (P2) learns a collection of transforms and a clustering for the image patches, together with the patches' sparse coefficients $\{\mathbf{Z}_i\}$. The next section uses these transforms for image reconstruction.

C. LDCT Reconstruction with ULTRA Regularization

We propose a PWLS-ULTRA framework, where we solve (P1) but with the regularizer $\mathsf{R}(\mathbf{x})$ defined based on a union

of sparsifying transforms as

$$\mathsf{R}(\mathbf{x}) \triangleq \min_{\{\mathbf{z}_j, C_k\}} \sum_{k=1}^{K} \Big\{ \sum_{j \in C_k} \big\{ \tau_j \|\mathbf{\Omega}_k \mathbf{P}_j \mathbf{x} - \mathbf{z}_j\|_2^2 + \gamma^2 \|\mathbf{z}_j\|_0 \big\} \Big\} \quad \text{s.t.} \quad \{C_k\} \in \mathcal{G}. \tag{3}$$

This regularizer measures the sparsification error of each patch for its best-matched transform. Using (3), (P1) estimates the image $\mathbf{x}$, the sparse coefficients of image patches $\{\mathbf{z}_j\}$, and the cluster assignments $\{C_k\}$ from LDCT sinogram data $\mathbf{y}$.

III. Algorithms and Properties

The square transform learning and the PWLS-ST formulations are special cases (corresponding to $K = 1$) of the ULTRA-based formulations. Therefore, this section describes algorithms for solving (P1) with regularizer (3) and (P2).

A. Algorithm for Training a Union of Transforms

We adopt an alternating minimization algorithm for (P2) that alternates between a *transform update step* (solving for $\{\mathbf{\Omega}_k\}$) and a *sparse coding and clustering step* (solving for $\{\mathbf{Z}_i, C_k\}$). These steps are described next.

1) Transform Update Step: With $\{\mathbf{Z}_i, C_k\}$ fixed, we solve the following optimization problem for $\{\mathbf{\Omega}_k\}$ [38]:

$$\min_{\{\mathbf{\Omega}_k\}} \sum_{k=1}^{K} \sum_{i \in C_k} \|\mathbf{\Omega}_k \mathbf{X}_i - \mathbf{Z}_i\|_2^2 + \sum_{k=1}^{K} \lambda_k Q(\mathbf{\Omega}_k). \tag{4}$$

Since the objective is in summation form, the above problem separates into K independent single transform learning problems that we solve in parallel. The kth such optimization problem is as follows:

$$\min_{\mathbf{\Omega}_k} \sum_{i \in C_k} \|\mathbf{\Omega}_k \mathbf{X}_i - \mathbf{Z}_i\|_2^2 + \lambda_k Q(\mathbf{\Omega}_k). \tag{5}$$

We update the transform $\mathbf{\Omega}_k$ following prior work [30], [38]. Let $\mathbf{Q}\mathbf{\Sigma}\mathbf{R}^T$ denote the full singular value decomposition of $\mathbf{L}^{-1}\mathbf{X}_{C_k}\mathbf{Z}_{C_k}^T$, with $\mathbf{L}\mathbf{L}^T \triangleq \mathbf{X}_{C_k}\mathbf{X}_{C_k}^T + \lambda_k \mathbf{I}$ (i.e., $\mathbf{L}$ is a matrix square root). Then, the minimizer of (5) is

$$\hat{\mathbf{\Omega}}_k = 0.5\mathbf{R}\big(\mathbf{\Sigma} + (\mathbf{\Sigma}^2 + 2\lambda_k \mathbf{I})^{\frac{1}{2}}\big)\mathbf{Q}^T \mathbf{L}^{-1}. \tag{6}$$

2) Sparse Coding and Clustering Step: With $\{\mathbf{\Omega}_k\}$ fixed, we solve the following sub-problem for $\{\mathbf{Z}_i, C_k\}$:

$$\min_{\{\mathbf{Z}_i, C_k\}} \sum_{k=1}^{K} \sum_{i \in C_k} \Big\{ \|\mathbf{\Omega}_k \mathbf{X}_i - \mathbf{Z}_i\|_2^2 + \eta^2 \|\mathbf{Z}_i\|_0 + \lambda_0 \|\mathbf{X}_i\|_2^2 Q(\mathbf{\Omega}_k) \Big\} \tag{7}$$

For given cluster memberships, the optimal sparse codes are $\mathbf{Z}_i = H_\eta(\mathbf{\Omega}_k \mathbf{X}_i), \forall i \in C_k$, where the *hard-thresholding* operator $H_\eta(\cdot)$ zeros out vector entries with magnitude less than η. Using this result, it follows that the optimal cluster membership for each $\mathbf{X}_i$ in (7) is $\hat{k}_i = \underset{1 \le k \le K}{\arg\min} \big\{ \|\mathbf{\Omega}_k \mathbf{X}_i - H_\eta(\mathbf{\Omega}_k \mathbf{X}_i)\|_2^2 + \eta^2 \|H_\eta(\mathbf{\Omega}_k \mathbf{X}_i)\|_0 + \lambda_0 \|\mathbf{X}_i\|_2^2 Q(\mathbf{\Omega}_k) \big\}$, and the corresponding optimal sparse code is $\hat{\mathbf{Z}}_i = H_\eta(\mathbf{\Omega}_{\hat{k}_i} \mathbf{X}_i)$.

B. PWLS-ULTRA Image Reconstruction Algorithm

We propose an alternating algorithm for the PWLS-ULTRA formulation (i.e., (P1) with regularizer (3)) that alternates between updating $\mathbf{x}$ (*image update step*), and $\{\mathbf{z}_j, C_k\}$ (*sparse coding and clustering step*).

1) Image Update Step: With $\{\mathbf{z}_j, C_k\}$ fixed, (P1) for PWLS-ULTRA reduces to the following weighted least squares problem:

$$\min_{\mathbf{x} \succeq \mathbf{0}} \frac{1}{2} \|\mathbf{y} - \mathbf{A}\mathbf{x}\|_{\mathbf{W}}^2 + \mathsf{R}_2(\mathbf{x}) \tag{8}$$

where $\mathsf{R}_2(\mathbf{x}) \triangleq \beta \sum_{k=1}^{K} \sum_{j \in C_k} \tau_j \|\mathbf{\Omega}_k \mathbf{P}_j \mathbf{x} - \mathbf{z}_j\|_2^2$.

We solve (8) using the recent relaxed OS-LALM [44], whose iterations are shown in Algorithm 1. For each iteration n, we further iterate over $1 \le m \le M$ corresponding to M ordered subsets. The matrices $\mathbf{A}_m$, $\mathbf{W}_m$, and the vector $\mathbf{y}_m$ are sub-matrices of $\mathbf{A}$, $\mathbf{W}$, and sub-vector of $\mathbf{y}$, respectively, for the mth subset. $\mathbf{D}_\mathbf{A} \succeq \mathbf{A}^T\mathbf{W}\mathbf{A}$ is a diagonal majorizing matrix of $\mathbf{A}^T\mathbf{W}\mathbf{A}$; specifically we use [40]

$$\mathbf{D}_\mathbf{A} \triangleq \mathsf{diag}\{\mathbf{A}^T\mathbf{W}\mathbf{A}\mathbf{1}\} \succeq \mathbf{A}^T\mathbf{W}\mathbf{A}. \tag{9}$$

The gradient $\nabla \mathsf{R}_2(\mathbf{x}) = 2\beta \sum_{k=1}^{K} \sum_{j \in C_k} \tau_j \mathbf{P}_j^T \mathbf{\Omega}_k^T (\mathbf{\Omega}_k \mathbf{P}_j \mathbf{x} - \mathbf{z}_j)$, the (over-)relaxation parameter $\alpha \in [1, 2)$, and the parameter $\rho > 0$ decreases gradually with iteration [44],

$$\rho_r(\alpha) = \begin{cases} 1, & r = 0 \\ \frac{\pi}{\alpha(r+1)} \sqrt{1 - \left(\frac{\pi}{2\alpha(r+1)}\right)^2}, & \text{otherwise,} \end{cases} \tag{10}$$

where r indexes the total number of n and m iterations. Lastly, $\mathbf{D}_\mathsf{R}$ in Algorithm 1 is a diagonal majorizing matrix of the Hessian of the regularizer $\mathsf{R}_2(\mathbf{x})$, specifically:

$$\begin{aligned} \mathbf{D}_\mathsf{R} &\triangleq 2\beta \Big\{ \max_k \lambda_{\max}(\mathbf{\Omega}_k^T \mathbf{\Omega}_k) \Big\} \sum_{k=1}^{K} \sum_{j \in C_k} \tau_j \mathbf{P}_j^T \mathbf{P}_j \\ &\succeq 2\beta \sum_{k=1}^{K} \sum_{j \in C_k} \tau_j \mathbf{P}_j^T \mathbf{\Omega}_k^T \mathbf{\Omega}_k \mathbf{P}_j = \nabla^2 \mathsf{R}_2(\mathbf{x}). \end{aligned} \tag{11}$$

Since this $\mathbf{D}_\mathsf{R}$ is independent of $\mathbf{x}$, $\{\mathbf{z}_j\}$, and $\{C_k\}$, we precompute it using patch-based operations [50] (cf. the supplement for details) prior to iterating.

2) Sparse Coding and Clustering Step: With $\mathbf{x}$ fixed, we solve the following sub-problem to determine the optimal sparse codes and cluster assignments for each patch:

$$\min_{\{\mathbf{z}_j\}, \{C_k\} \in \mathcal{G}} \sum_{k=1}^{K} \Big\{ \sum_{j \in C_k} \big\{ \tau_j \|\mathbf{\Omega}_k \mathbf{P}_j \mathbf{x} - \mathbf{z}_j\|_2^2 + \gamma^2 \|\mathbf{z}_j\|_0 \big\} \Big\}. \tag{12}$$

For each patch $\mathbf{P}_j\mathbf{x}$, with (optimized) $\mathbf{z}_j = H_{\tilde{\gamma}}(\mathbf{\Omega}_k \mathbf{P}_j \mathbf{x})$ and $\tilde{\gamma}_j \triangleq \gamma / \sqrt{\tau_j}$, the optimal cluster assignment is as follows:

$$\hat{k}_j = \underset{1 \le k \le K}{\arg\min} \|\mathbf{\Omega}_k \mathbf{P}_j \mathbf{x} - H_{\tilde{\gamma}_j}(\mathbf{\Omega}_k \mathbf{P}_j \mathbf{x})\|_2^2 + \frac{\gamma^2}{\tau_j} \|H_{\tilde{\gamma}_j}(\mathbf{\Omega}_k \mathbf{P}_j \mathbf{x})\|_0 \tag{13}$$

Minimizing over k finds the best-matched transform. Then, the optimal sparse codes are $\hat{\mathbf{z}}_j = H_{\tilde{\gamma}_j}(\mathbf{\Omega}_{\hat{k}_j} \mathbf{P}_j \mathbf{x})$.

3) Overall Algorithm: The proposed method for the PWLS-ULTRA problem is shown in Algorithm 1. The algorithm for the PWLS-ST formulation is obtained by setting $K = 1$ and skipping the clustering procedure in the sparse coding and clustering step. Algorithm 1 uses an initial image estimate and the union of pre-learned transforms $\{\mathbf{\Omega}_k\}$. It then alternates between the image update, and sparse coding and clustering step until a convergent criterion (such as $\|\tilde{\mathbf{x}}^{(t+1)} - \tilde{\mathbf{x}}^{(t)}\|_2 < \epsilon$ for some small $\epsilon > 0$) is satisfied, or alternatively until some maximum inner/outer iteration counts are reached.

Algorithm 1 PWLS-ULTRA Algorithm

Input: initial image $\tilde{\mathbf{x}}^{(0)}$, pre-learned $\{\mathbf{\Omega}_k\}$, thresholds $\{\tilde{\gamma}_j\}$, $\alpha = 1.999$, $\mathbf{D_A}$ in (9), $\mathbf{D_R}$ in (11), number of outer iterations T, number of inner iterations N, and number of subsets M.

Output: reconstructed image $\tilde{\mathbf{x}}^{(T)}$, cluster indices $\{\tilde{C}_k^{(T)}\}$.

for $t = 0, 1, 2, \cdots, T-1$ **do**

1) Image Update: $\{\tilde{\mathbf{z}}_j^{(t)}\}$ and $\{\tilde{C}_k^{(t)}\}$ fixed,

Initialization: $\rho = 1$, $\mathbf{x}^{(0)} = \tilde{\mathbf{x}}^{(t)}$, $\mathbf{g}^{(0)} = \boldsymbol{\zeta}^{(0)} = M\mathbf{A}_M^T\mathbf{W}_M(\mathbf{A}_M\mathbf{x}^{(0)} - \mathbf{y}_M)$ and $\mathbf{h}^{(0)} = \mathbf{D_A}\mathbf{x}^{(0)} - \boldsymbol{\zeta}^{(0)}$.

for $n = 0, 1, 2, \cdots, N-1$ **do**

for $m = 0, 1, 2, \cdots, M-1$ **do** $r = nM + m$

$$\begin{cases} \mathbf{s}^{(r+1)} = \rho(\mathbf{D_A}\mathbf{x}^{(r)} - \mathbf{h}^{(r)}) + (1-\rho)\mathbf{g}^{(r)} \\ \mathbf{x}^{(r+1)} = [\mathbf{x}^{(r)} - (\rho\mathbf{D_A} + \mathbf{D_R})^{-1}(\mathbf{s}^{(r+1)} + \nabla \mathsf{R}_2(\mathbf{x}^{(r)}))]_+ \\ \boldsymbol{\zeta}^{(r+1)} \triangleq M\mathbf{A}_m^T\mathbf{W}_m(\mathbf{A}_m\mathbf{x}^{(r+1)} - \mathbf{y}_m) \\ \mathbf{g}^{(r+1)} = \frac{\rho}{\rho+1}(\alpha\boldsymbol{\zeta}^{(r+1)} + (1-\alpha)\mathbf{g}^{(r)}) + \frac{1}{\rho+1}\mathbf{g}^{(r)} \\ \mathbf{h}^{(r+1)} = \alpha(\mathbf{D_A}\mathbf{x}^{(r+1)} - \boldsymbol{\zeta}^{(r+1)}) + (1-\alpha)\mathbf{h}^{(r)} \end{cases}$$

decreasing ρ using (10).

end for

end for

$\tilde{\mathbf{x}}^{(t+1)} = \mathbf{x}^{(NM)}$.

2) Sparse Coding and Clustering: with $\tilde{\mathbf{x}}^{(t+1)}$ fixed, for each $1 \leq j \leq N$, obtain $\hat{k}_j$ using (13). Then $\tilde{\mathbf{z}}_j^{(t+1)} = H_{\tilde{\gamma}_j}(\mathbf{\Omega}_{\hat{k}_j}\mathbf{P}_j\tilde{\mathbf{x}}^{(t+1)})$, and update $\tilde{C}_{\hat{k}_j}^{(t+1)}$.

end for

4) Computational Cost: Each outer iteration of the proposed Algorithm 1 involves the image update, and the sparse coding and clustering step. The cost of the sparse coding and clustering step scales as $O(l^2N)$ and is dominated by matrix-vector products. Importantly, unlike prior dictionary learning-based works [25], where the computations for the sparse coding step (involving orthogonal matching pursuit (OMP) [51]) can scale worse as $O(l^3N)$ (assuming synthesis sparsity levels of patches $\propto l$), the exact sparse coding and clustering in PWLS-ULTRA is cheaper [38], especially for large patch sizes. Similar to prior works [25], the computations in the image update step are dominated by the forward and backward projection operations. Section IV compares the proposed LDCT reconstruction methods to synthesis dictionary learning-based approaches, and shows that our transform approach runs faster and performs better.

IV. Experimental Results

This section presents experimental results illustrating properties of the proposed algorithms and demonstrating their promising performance for LDCT reconstruction compared to numerous recent methods. We include additional experimental results in the supplement.

A. Framework and Data

We evaluate the proposed PWLS-ULTRA and PWLS-ST (i.e., with $K = 1$) methods for 2D fan-beam and 3D axial cone-beam CT reconstruction of the XCAT phantom [48]. We also apply the proposed methods to low-dose (clinical) helical CT data of the chest.

Section IV-B illustrates the properties of the transform learning and image reconstruction methods. Sections IV-C and IV-D show results for 2D fan-beam and 3D axial cone-beam CT, respectively, for the XCAT phantom data. We used the "Poisson + Gaussian" model, i.e., $y_i \sim \tilde{k}\,\text{Poisson}\{I_0 \exp(-[\mathbf{Ax}]_i)\} + \text{Normal}\{0, \sigma^2\}$ to simulate CT measurements of the XCAT phantom, where I_0 is the incident X-ray intensity incorporating X-ray source illumination and the detector gain, the parameter $\tilde{k} = 1000$ models the conversion gain from X-ray photons to electrons, and $\sigma^2 = 330^2$ is the variance of electronic noise [52]. We compare the image reconstruction quality obtained with PWLS-ST and PWLS-ULTRA with those of:

- **FBP**: conventional FBP method with a Hanning window.
- **PWLS-EP**: PWLS reconstruction with the edge-preserving regularizer $\mathsf{R}(\mathbf{x}) = \sum_{j=1}^{N_p}\sum_{k\in N_j}\kappa_j\kappa_k\varphi(x_j - x_k)$, where N_j is the size of the neighborhood, κ_j and κ_k are the parameters encouraging uniform resolution (used in 2D) or uniform noise (used in 3D) [47], and $\varphi(t) \triangleq \delta^2\left(\sqrt{1 + |t/\delta|^2} - 1\right)$ for 2D, $\varphi(t) \triangleq \delta^2(|t/\delta| - \log(1 + |t/\delta|))$ ($\delta = 10$ HU) for 3D. We optimized this cost function using the relaxed OS-LALM [44].
- **PWLS-DL**: PWLS reconstruction with a learned over-complete synthesis dictionary based regularization, whose image update step is optimized by relaxed OS-LALM instead of SQS-OS used in [25].

Section IV-E reports the reconstructions from low-dose helical CT (clinical) data of the chest. Finally, Section IV-F compares the performance of PWLS-ULTRA to an oracle scheme that uses cluster memberships estimated directly from the reference or ground truth images.

To compare various methods quantitatively for the case of the XCAT phantom, we calculated the Root Mean Square Error (RMSE) and Structural Similarity Index Measurement (SSIM) [49] of the reconstructions in a region of interest (ROI). RMSE in Hounsfield units (HU) is defined as RMSE $= \sqrt{\sum_{i=1}^{N_{p,\text{ROI}}}(\hat{x}_i - x_i^*)^2/N_{p,\text{ROI}}}$, where $\mathbf{x}^*$ is the ground truth image and $N_{p,\text{ROI}}$ is the number of pixels (voxels) in the ROI. Unless otherwise noted, we tuned the parameters of various methods for each experiment to achieve the lowest RMSE. For the clinical low-dose chest data, the reconstructions are evaluated visually. We display all reconstructions in this section using a display window $[800, 1200]$ HU, unless otherwise noted.

In the 2D fan-beam CT experiments, we pre-learned square transforms and union of square transforms from 8×8 image patches extracted from five 512×512 XCAT phantom slices, with a patch stride 1×1. We ran 1000 iterations of the alternating minimization (transform learning) algorithm in Section III-A (or in [30] for $K = 1$) to ensure convergence, and used $\lambda_0 = 31$. The transforms were initialized with the 2D DCT, and k-means clustering (of patches) was used to initialize the clusters for learning a union of transforms. We simulated a 2D fan-beam CT scan using a 1024×1024 XCAT phantom slice that differs from the training slices,

and $\Delta_x = \Delta_y = 0.4883$ mm. Noisy sinograms of size 888×984 were numerically simulated with GE LightSpeed fan-beam geometry corresponding to a monoenergetic source with 1×10^4 and 5×10^3 incident photons per ray and no scatter, respectively. We reconstructed a 512×512 image with a coarser grid, where $\Delta_x = \Delta_y = 0.9766$ mm. The ROI here was a circular (around center) region containing all the phantom tissues.

In the 3D cone-beam CT reconstruction experiments, we pre-learned STs and union of square transforms from $8 \times 8 \times 5$ or $8 \times 8 \times 8$ patches ($N' \approx 1 \times 10^6$) extracted from a $420 \times 420 \times 54$ XCAT phantom with a patch stride $2 \times 2 \times 2$. We ran the alternating minimization transform learning algorithms for 1000 iterations with $\lambda_0 = 31$. The transforms were initialized with the 3D DCT, and a random initialization was used for the clusters (because k-means produced some empty clusters for large K) for learning a union of square transforms. We simulated an axial cone-beam CT scan using a $840 \times 840 \times 96$ XCAT phantom with $\Delta_x = \Delta_y = 0.4883$ mm and $\Delta_z = 0.625$ mm. We generated sinograms of size $888 \times 64 \times 984$ using GE LightSpeed cone-beam geometry corresponding to a monoenergetic source with 1×10^4 and 5×10^3 incident photons per ray and no scatter, respectively. We reconstructed a $420 \times 420 \times 96$ volume with a coarser grid, where $\Delta_x = \Delta_y = 0.9766$ mm and $\Delta_z = 0.625$ mm. The ROI for the 3D case consisted of the central 64 of 96 axial slices and a circular (around center) region in each slice (cylinder in 3D).

For the clinical data, we reconstructed a $420 \times 420 \times 222$ image volume with patch size $8 \times 8 \times 8$ and patch stride $3 \times 3 \times 3$ ($\tilde{N} \approx 1.5 \times 10^6$ patches), where $\Delta_x = \Delta_y = 1.1667$ mm and $\Delta_z = 0.625$ mm, from a chest region helical CT (low-dose) scan. The size of the sinogram was $888 \times 64 \times 3611$ and pitch 1.0 (about 3.7 rotations with rotation time 0.4 seconds). The tube current and tube voltage of the X-ray source were 750 mA and 120 kVp, respectively.

B. Behavior of the Learning and PWLS-ULTRA Algorithms

We evaluate the behavior of the PWLS-ULTRA method for 3D cone-beam CT data with $I_0 = 1 \times 10^4$. Fig. 2 shows the central slices along three directions for the underlying (true) XCAT phantom volume. We reconstruct this volume from low-dose CT measurements. Fig. 2 also shows the RMSE and SSIM of PWLS-ULTRA for various choices of K, the number of clusters (patch size $8 \times 8 \times 8$ and patch stride $2 \times 2 \times 2$). Rich models (large K) produce better reconstructions compared to using a single ST ($K = 1$). For the piece-wise constant phantom, $K = 5$ clusters works well enough, with only a small additional RMSE or SSIM improvement observed for larger K. Larger values of K led to sharper image edges.

Fig. 3 presents an example of the pixel-level clustering (in the central axial slice) achieved with the PWLS-ULTRA method for $K = 5$. Since PWLS-ULTRA clusters image patches, we cluster individual pixels using a majority vote among the (3D) patches that overlap the pixel. Class 1 contains most of the soft tissues; Class 2 comprises most of the bones and blood vessels; classes 3 and 4 have some high-contrast edges oriented along specific directions; and Class 5 mainly includes low-contrast edges. Since the clustering step (during both training and reconstruction) is unsupervised, i.e., different anatomical structures were not labeled manually, there are also a few edges with high pixel intensities included in Class 2. The trained (3D) transforms (with $\eta = 50$) for each cluster are also displayed in a similar manner as in Fig. 1. The transforms show features (e.g., with specific orientations) that clearly reflect the properties of the patches/tissues in each class.

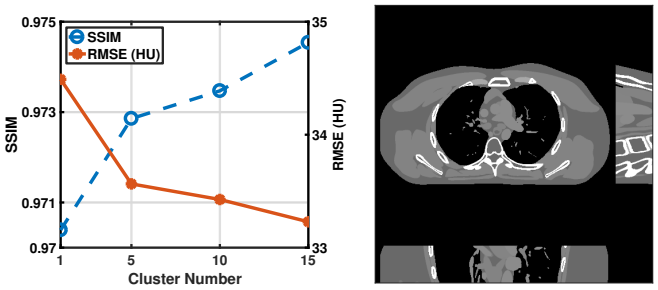

Fig. 2. RMSE and SSIM for PWLS-ULTRA for various choices of number of clusters K (left), and the central slices along three directions for the underlying volume in the cone-beam CT reconstruction experiments (right).

C. 2D LDCT Reconstruction Results and Comparisons

1) Reconstruction Quality: We evaluate the performance of various algorithms for image reconstruction from low-dose fan-beam CT data. Initialized with FBP reconstructions, we ran the PWLS-EP algorithm for 50 iterations using relaxed OS-LALM with 20 subsets, and using regularization parameter $\beta = 2^{7.3}$ and $\beta = 2^{8.0}$ for $I_0 = 1 \times 10^4$ and $I_0 = 5 \times 10^3$, respectively. For PWLS-DL, PWLS-ST, and PWLS-ULTRA, we initialized with the PWLS-EP reconstruction, and ran 200 outer iterations with 10 iterations of the image update step without ordered subsets, i.e., $N = 10$, $M = 1$. For PWLS-DL, we pre-learned a 64×256 overcomplete dictionary from 8×8 patches extracted from five XCAT phantom slices (same slices as used for transform learning) with a patch stride 1×1, using a maximum patch-wise sparsity level of 20 and an error threshold or tolerance for sparse coding of 10^{-3}. During reconstruction, we used a regularization parameter of 3.5×10^7, and a maximum sparsity level of 25, and chose error tolerances as 70 and 75 for $I_0 = 1 \times 10^4$ and $I_0 = 5 \times 10^3$, respectively. For PWLS-ST and PWLS-ULTRA ($K = 15$), we set $\gamma = 35$, and chose (β, η) for the two incident photon intensities as follows: $(7.0 \times 10^7, 110)$ and $(5.0 \times 10^7, 110)$ for PWLS-ST; and $(9.0 \times 10^7, 110)$ and $(7.0 \times 10^7, 125)$ for PWLS-ULTRA. We ran the proposed methods without the patch-based weights (i.e., $\tau_j = 1$, $\forall\ j$ in (2)), which worked well in the 2D imaging experiments. For PWLS-ULTRA, we performed the clustering step only once every 10 outer iterations, which worked well and reduced runtimes. We updated the sparse codes of the patches in every outer iteration.

Table I lists the RMSE and SSIM values for reconstructions with FBP, PWLS-EP, PWLS-DL, PWLS-ST, and PWLS-ULTRA ($K = 15$). The adaptive PWLS methods outperform the conventional FBP and the non-adaptive PWLS-EP. At $I_0 = 1 \times 10^4$, PWLS-ST achieves similar reconstruction quality as PWLS-DL that uses an overcomplete dictionary. However, PWLS-DL outperforms PWLS-ST for a lower dose.

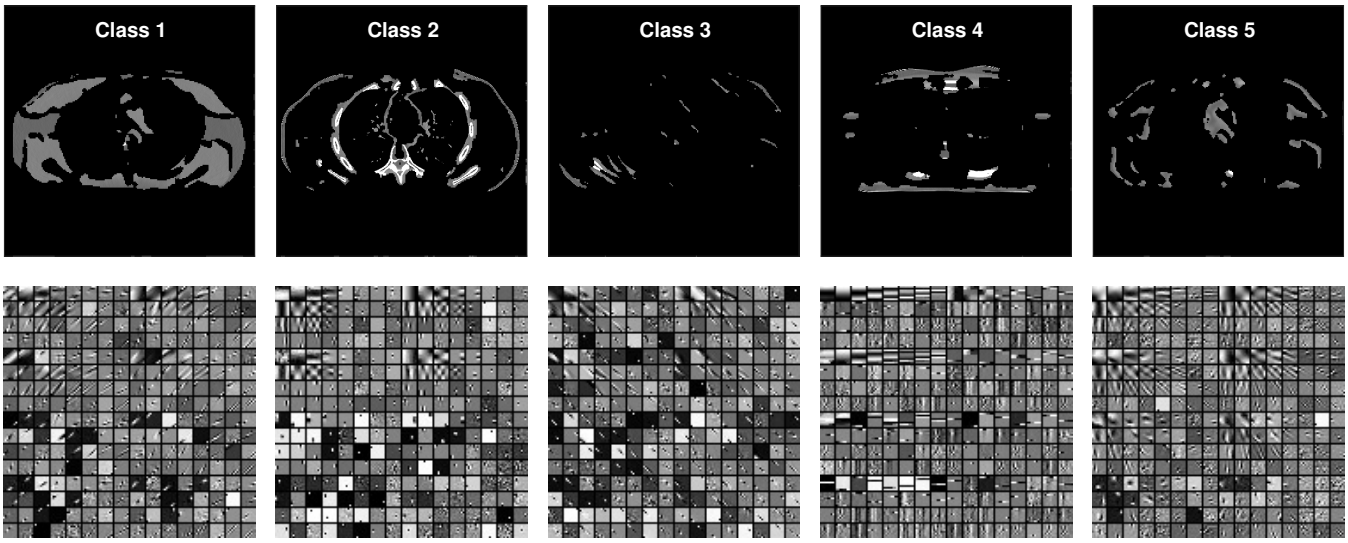

Fig. 3. Pixel-level clustering results (top row) for the central axial slice of the PWLS-ULTRA ($K = 5$) reconstruction at $I_0 = 1 \times 10^4$. The pixels in each class are displayed using the intensities in the reconstruction. The corresponding transforms are in the bottom row.

TABLE I
RMSE (HU) AND SSIM OF 2D (FAN-BEAM) IMAGE RECONSTRUCTIONS WITH FBP, PWLS-EP, PWLS-DL, PWLS-ST, AND PWLS-ULTRA ($K = 15$) FOR TWO INCIDENT PHOTON INTENSITIES.

Intensity	FBP	EP	DL	ST	ULTRA
1×10^4	69.5	24.6	21.3	21.9	**19.0**
	0.361	0.900	0.954	0.953	**0.960**
5×10^3	78.1	30.8	25.1	26.9	**23.9**
	0.323	0.878	0.949	0.941	**0.951**

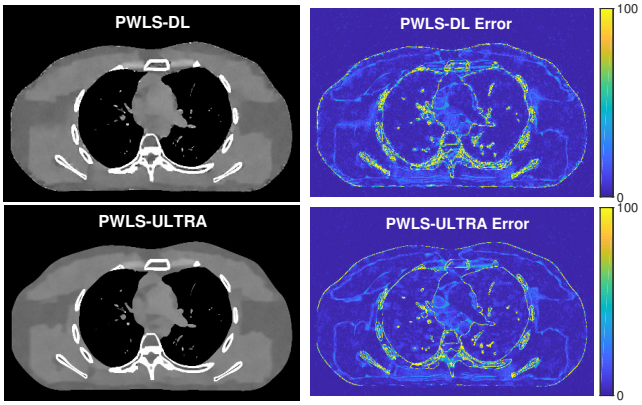

Fig. 4. Comparison of 2D reconstructions (cropped) and reconstruction errors (magnitudes) for PWLS-DL and PWLS-ULTRA ($K = 15$) at $I_0 = 1 \times 10^4$.

Importantly, PWLS-ULTRA using a union of learned transforms leads to better reconstruction quality than both PWLS-DL and PWLS-ST. Fig. 4 compares the reconstructions and reconstruction errors (relative to the ground truth in Fig. 5) for PWLS-DL and PWLS-ULTRA. The ULTRA reconstruction has fewer artifacts and soft tissue edge clarity.

2) Runtimes: To compare the runtimes of various data-driven methods, we ran PWLS-DL, PWLS-ST, and PWLS-ULTRA ($K = 15$) (all initialized with the FBP reconstruction) for 200 outer iterations with 3 iterations of the image update step and 3 ordered subsets. Fig. 5 shows the RMSE converging quickly for various methods, with faster convergence for the

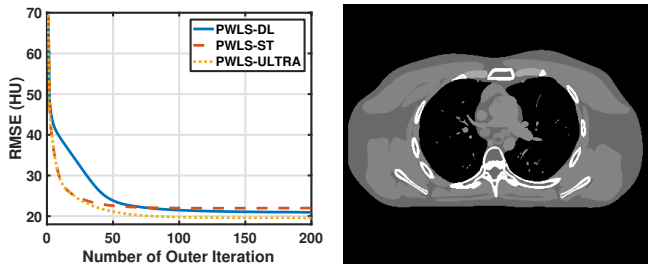

Fig. 5. RMSE vs. outer iterations (left) for PWLS-DL, PWLS-ST and PWLS-ULTRA ($K = 15$) at $I_0 = 1 \times 10^4$, and the reference image (cropped for display) for the 2D fan-beam CT experiment (right).

proposed PWLS-ST and PWLS-ULTRA schemes. While the total runtime for the 200 iterations (using a machine with two 2.80 GHz 10-core Intel Xeon E5-2680 processors) was 110 minutes for PWLS-DL, it was only 56 minutes for PWLS-ST and 60 minutes for PWLS-ULTRA. The runtime of PWLS-DL was quite equally dominated by the sparse coding (with OMP [51]) and image update steps, whereas for the transform-based methods, the sparse coding and clustering involving simple closed-form solutions and thresholding operations required negligible runtime. The advantage in runtime was achieved despite using an unoptimized Matlab implementation of PWLS-ST and PWLS-ULTRA, and using an efficient MEX/C implementation for sparse coding with OMP [51] in PWLS-DL. PWLS-DL is far slower for 3D reconstructions with large 3D patches. Hence, we focus our comparisons between the transform learning and dictionary learning-based schemes for 2D LDCT reconstruction.

D. Low-dose Cone-beam CT Results and Comparisons

We evaluate the performance of various algorithms for reconstructing CT volumes from simulated low-dose cone-beam (3D) CT data. Initialized with FDK reconstructions, we ran the PWLS-EP algorithm with regularization parameter $\beta = 2^{19.5}$ for 50 and 100 iterations with 24 and 12 subsets for $I_0 = 1 \times 10^4$ and $I_0 = 5 \times 10^3$, respectively. We evaluate PWLS-ST and PWLS-ULTRA without the patch-based

TABLE II
RMSE (HU) AND SSIM OF 3D (CONE-BEAM) RECONSTRUCTIONS WITH FDK, PWLS-EP, PWLS-ST, PWLS-ULTRA ($K = 15$), AND PWLS-ULTRA ($K = 15$) WITH PATCH-BASED WEIGHTS (τ_j), FOR TWO INCIDENT PHOTON INTENSITIES.

Intensity	FDK	EP	ST	ULTRA	ULTRA-$\{\tau_j\}$
1×10^4	67.5	38.8	34.5	33.4	**33.0**
	0.476	0.946	0.970	0.974	**0.977**
5×10^3	136.5	46.3	39.4	38.7	**37.9**
	0.420	0.933	0.961	0.967	**0.969**

weights. We also evaluate PWLS-ULTRA with such weights. For PWLS-ST and PWLS-ULTRA, the patch size was $8 \times 8 \times 5$ with a patch stride $2 \times 2 \times 2$ ($\tilde{N} \approx 2 \times 10^6$ patches). Initialized with the PWLS-EP reconstruction, we ran 2 iterations of the image update step with 4 subsets. We performed the clustering step once every 50 outer iterations, which worked well and saved computation. We learned transforms with $\eta = 100$, and chose (β, γ) for $I_0 = 1 \times 10^4$ and $I_0 = 5 \times 10^3$ as follows: $(1.5 \times 10^8, 20)$ and $(9.0 \times 10^7, 20)$ for PWLS-ST ($\tau_j = 1$); $(2.0 \times 10^8, 20)$ and $(1.2 \times 10^8, 20)$ for PWLS-ULTRA ($\tau_j = 1$); and $(5.0 \times 10^5, 400)$ and $(3.5 \times 10^5, 400)$ for PWLS-ULTRA with the patch-based weights τ_j.

Table II lists the RMSE and SSIM values of the reconstructions with FDK, PWLS-EP, PWLS-ST ($\tau_j = 1$), PWLS-ULTRA ($K = 15$, $\tau_j = 1$), and PWLS-ULTRA ($K = 15$) with patch-based weights τ_j. Both PWLS-ST and PWLS-ULTRA significantly improve the RMSE and SSIM compared to FDK and the non-adaptive PWLS-EP. Importantly, PWLS-ULTRA with a richer union of learned transforms leads to better reconstructions than PWLS-ST with a single learned ST. Incorporating the patch-based weights in PWLS-ULTRA leads to further improvement in reconstruction quality compared to PWLS-ULTRA with uniform weights $\tau_j = 1$ for all patches. In particular, the patch-based weights lead to improved resolution for soft tissues in 3D LDCT reconstructions.

Fig. 6 shows the reconstructions and the corresponding error (magnitudes) images (shown for the central axial, sagittal, and coronal planes) for FDK, PWLS-EP, and PWLS-ULTRA ($K = 15$) with the patch-based weights. Compared to FDK and PWLS-EP, PWLS-ULTRA significantly improves image quality by reducing noise and preserving structural details. Since the PWLS-ULTRA parameters were chosen to achieve lowest overall RMSE (in entire ROI), the reconstruction could potentially have some blurry components (e.g., in the central lung region). Resolution in a specific smaller ROI could be improved by tuning parameters with respect to that ROI. Fig. 7 shows the RMSE for each axial slice in the PWLS-EP and PWLS-ULTRA with patch-based weights reconstructions. PWLS-ULTRA clearly provides large improvements in RMSE for many slices, with greater improvements near the central slice.

E. Results for Clinical Data: Chest Scan

We reconstruct the chest volume from low-dose helical CT data. For PWLS-EP, we used the same parameter settings as used for this data in prior work [44]. Initializing with the PWLS-EP reconstruction, we ran the PWLS-ULTRA ($K = 5$)

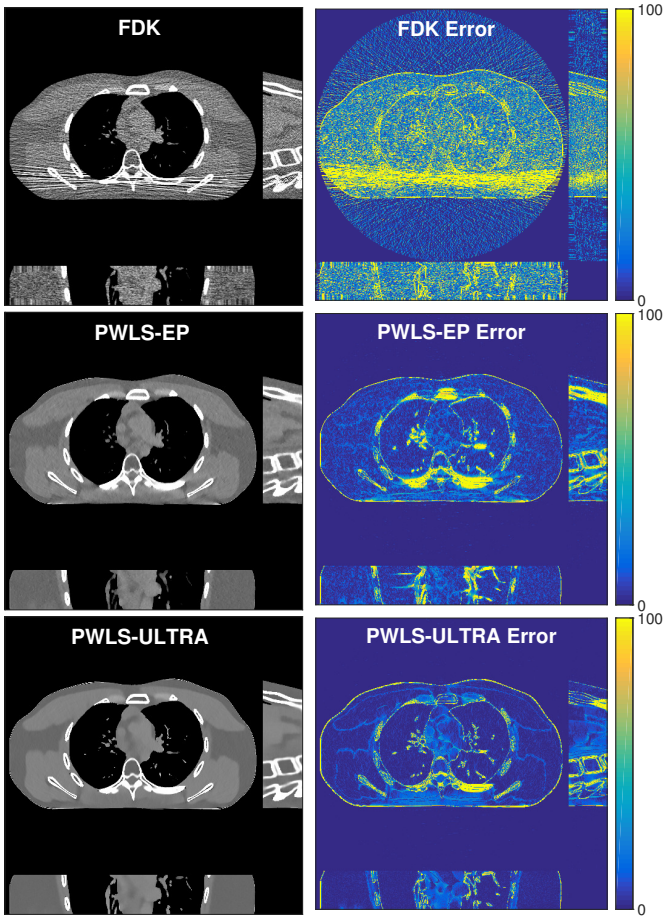

Fig. 6. Comparison of the reconstructions and corresponding error images (shown for the central axial, sagittal, and coronal planes) for FDK, PWLS-EP, and PWLS-ULTRA ($K = 15$) with patch-based weights at $I_0 = 1 \times 10^4$.

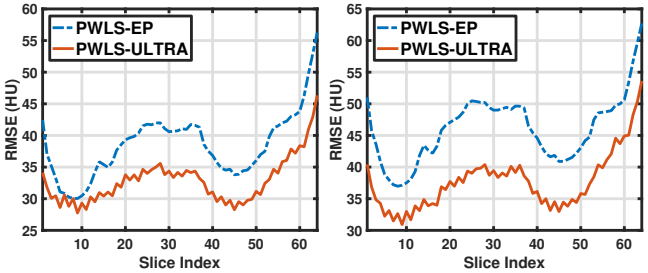

Fig. 7. RMSE of each axial slice in the PWLS-EP and PWLS-ULTRA reconstructions for $I_0 = 1 \times 10^4$ (left) and $I_0 = 5 \times 10^3$ (right).

method with the patch-based weights τ_j for 60 outer iterations with 3 iterations of the image update step and 4 subsets. We performed clustering once every 10 outer iterations. We chose $\beta = 2 \times 10^5$ and $\gamma = 400$ for PWLS-ULTRA (which are quite similar to the values for the XCAT phantom in Section IV-D) to obtain good visual quality of the reconstruction. We used the transforms learned from the XCAT phantom volume with $\eta = 100$ to obtain reconstructions with PWLS-ULTRA for the low-dose clinical chest CT data. The supplement shows that transforms learned from the XCAT phantom have similar types of features and provide similar visual reconstructions as transforms learned from the PWLS-EP reconstruction of the chest data. This suggests that the transform learning algorithm can extract quite general and effective image features without

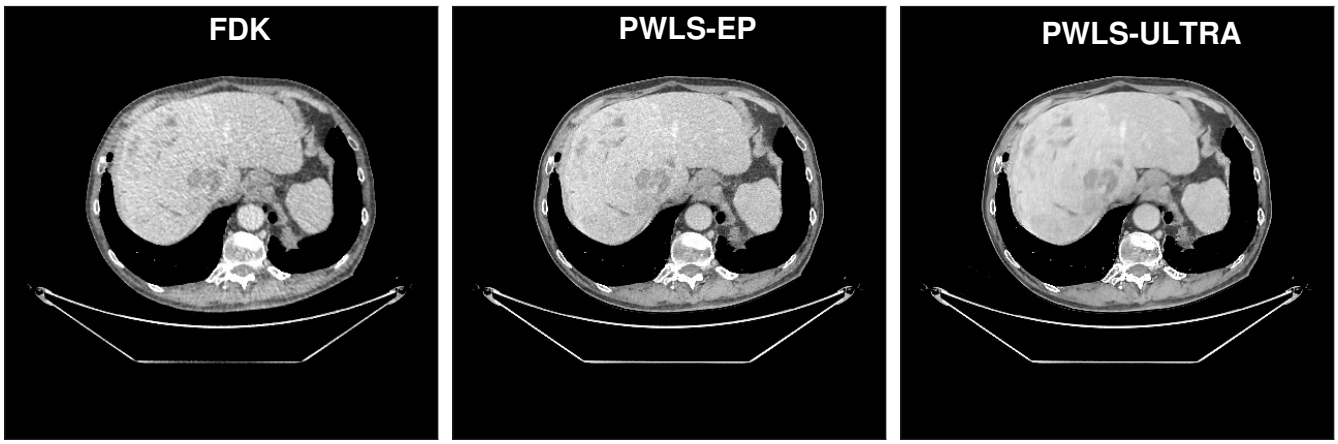

Fig. 8. Chest reconstructions (shown for central axial plane) from low-dose helical CT data, with the FDK, PWLS-EP, and PWLS-ULTRA ($K = 5$) methods.

requiring a very closely matched training dataset.

Fig. 8 shows the reconstructions (shown for the central axial plane in the 3D volume) for FDK (provided by GE Healthcare), PWLS-EP, and PWLS-ULTRA ($K = 5$). The PWLS-ULTRA reconstruction has lower artifacts and noise. Moreover, the image features and edges are better reconstructed by PWLS-ULTRA than by PWLS-EP or FDK.

F. Comparison to Oracle Clustering Scheme

We consider the 3D cone-beam CT data in Section IV-D with $I_0 = 1 \times 10^4$, and compare the PWLS-ULTRA ($K = 15$) method with patch-based weights to an oracle PWLS-ULTRA scheme, where the cluster memberships are pre-determined (and fixed during reconstruction) by performing the sparse coding and clustering step (with the learned transforms) on the patches of the reference or ground truth volume. The oracle scheme thus uses the best possible estimate of the cluster memberships. Otherwise, we used the same parameters for the two cases. Fig. 9 compares the reconstructions for the two cases. The proposed PWLS-ULTRA underperforms the oracle scheme by only 1.6 HU. The more precise clustering leads to sharper edges for the latter method. This also suggests that there is room for potentially improving the proposed clustering-based PWLS-ULTRA scheme, which could be pursued in future works.

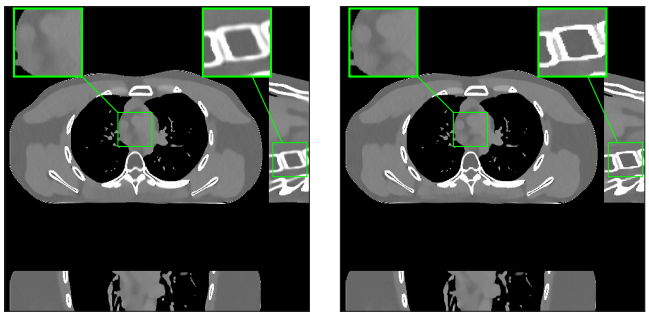

Fig. 9. Reconstruction with PWLS-ULTRA ($K = 15$) with weights τ_j (left) at $I_0 = 1 \times 10^4$, compared to the reconstruction with the oracle scheme (right), where the cluster memberships were pre-determined from the ground truth. RMSE and SSIM values of 33.0 and 0.977 (left), and 31.4 and 0.982 (right) respectively, for the volumes, indicates that more precise clustering can provide better reconstructions and sharper edges (see zoom-ins).

V. Conclusions

We presented the PWLS-ST and PWLS-ULTRA methods for low-dose CT imaging, combining conventional penalized weighted least squares reconstruction with regularization based on pre-learned sparsifying transforms. Experimental results with 2D and 3D axial CT scans of the XCAT phantom and 3D helical chest scans show that for low-dose levels, the proposed methods provide high quality image reconstructions compared to conventional techniques such as FBP or PWLS reconstruction with a nonadaptive edge-preserving regularizer. PWLS-ULTRA also outperforms PWLS-DL with a learned overcomplete dictionary and is also faster than the latter. Finally, the ULTRA scheme with a richer union of transforms model provides better reconstruction of various features such as bones, specific soft tissues, and edges, compared to the proposed PWLS-ST. We leave the investigation of convergence guarantees and automating the parameter selection for the proposed PWLS algorithms to future work. The field of transform learning is rapidly growing, and we hope to investigate new transform learning-based LDCT reconstruction methods, such as involving rotationally invariant transforms, or online transform learning [53], [54], etc., in future work.

VI. Acknowledgments

The authors thank GE Healthcare for supplying the helical chest data used in this work.

References

[1] L. A. Feldkamp, L. C. Davis, and J. W. Kress, "Practical cone beam algorithm," *J. Opt. Soc. Am. A*, vol. 1, pp. 612–619, June 1984.

[2] K. Imai, M. Ikeda, Y. Enchi, and T. Niimi, "Statistical characteristics of streak artifacts on CT images: Relationship between streak artifacts and mA s values," *Med. Phys.*, vol. 36, pp. 492–499, Feb. 2009.

[3] J. A. Fessler, "Statistical image reconstruction methods for transmission tomography," in *Handbook of Medical Imaging, Volume 2. Medical Image Processing and Analysis* (M. Sonka and J. M. Fitzpatrick, eds.), pp. 1–70, Bellingham: Proc. SPIE, 2000.

[4] I. A. Elbakri and J. A. Fessler, "Statistical image reconstruction for polyenergetic X-ray computed tomography," *IEEE Trans. Med. Imag.*, vol. 21, pp. 89–99, Feb. 2002.

[5] K. Sauer and C. Bouman, "A local update strategy for iterative reconstruction from projections," *IEEE Trans. Sig. Proc.*, vol. 41, no. 2, pp. 534–548.

[6] J.-B. Thibault, C. A. Bouman, K. D. Sauer, and J. Hsieh, "A recursive filter for noise reduction in statistical iterative tomographic imaging," in *Proc. SPIE*, vol. 6065, pp. 60650X–1–60650X–10, 2006.

[7] J.-B. Thibault, K. Sauer, C. Bouman, and J. Hsieh, "A three-dimensional statistical approach to improved image quality for multi-slice helical CT," *Med. Phys.*, vol. 34, pp. 4526–4544, Nov. 2007.

[8] A. M. Bruckstein, D. L. Donoho, and M. Elad, "From sparse solutions of systems of equations to sparse modeling of signals and images," *SIAM Review*, vol. 51, no. 1, pp. 34–81, 2009.

[9] R. Rubinstein, A. M. Bruckstein, and M. Elad, "Dictionaries for sparse representation modeling," *Proc. IEEE*, vol. 98, pp. 1045–1057, June 2010.

[10] B. A. Olshausen and D. J. Field, "Emergence of simple-cell receptive field properties by learning a sparse code for natural images," *Nature*, vol. 381, no. 6583, pp. 607–609, 1996.

[11] K. Engan, S. Aase, and J. Hakon-Husoy, "Method of optimal directions for frame design," in *Proc. IEEE International Conference on Acoustics, Speech, and Signal Processing*, pp. 2443–2446, 1999.

[12] M. Aharon, M. Elad, and A. Bruckstein, "K-SVD: an algorithm for designing overcomplete dictionaries for sparse representation," *IEEE Trans. Sig. Proc.*, vol. 54, pp. 4311–4322, Nov. 2006.

[13] M. Yaghoobi, T. Blumensath, and M. Davies, "Dictionary learning for sparse approximations with the majorization method," *IEEE Trans. Sig. Proc.*, vol. 57, no. 6, pp. 2178–2191, 2009.

[14] J. Mairal, F. Bach, J. Ponce, and G. Sapiro, "Online learning for matrix factorization and sparse coding," *J. Mach. Learn. Res.*, vol. 11, pp. 19–60, 2010.

[15] M. Elad and M. Aharon, "Image denoising via sparse and redundant representations over learned dictionaries," *IEEE Trans. Im. Proc.*, vol. 15, pp. 3736–3745, Dec. 2006.

[16] J. Mairal, M. Elad, and G. Sapiro, "Sparse representation for color image restoration," *IEEE Trans. Im. Proc.*, vol. 17, no. 1, pp. 53–69, 2008.

[17] M. Protter and M. Elad, "Image sequence denoising via sparse and redundant representations," *IEEE Trans. on Image Processing*, vol. 18, no. 1, pp. 27–36, 2009.

[18] S. Kong and D. Wang, "A dictionary learning approach for classification: Separating the particularity and the commonality," in *Proceedings of the 12th European Conference on Computer Vision*, pp. 186–199, 2012.

[19] S. Ravishankar and Y. Bresler, "MR image reconstruction from highly undersampled k-space data by dictionary learning," *IEEE Trans. Med. Imag.*, vol. 30, no. 5, pp. 1028–1041, 2011.

[20] Y. Chen, X. Yin, L. Shi, H. Shu, L. Luo, J.-L. Coatrieux, and C. Toumoulin, "Improving abdomen tumor low-dose CT images using a fast dictionary learning based processing," *Phys. Med. Biol.*, vol. 58, pp. 5803–5820, Aug. 2013.

[21] Y. Lu, J. Zhao, and G. Wang, "Few-view image reconstruction with dual dictionaries," *Phys. Med. Biol.*, vol. 57, pp. 173–190, Jan. 2012.

[22] W. Zhou, J.-F. Cai, and H. Gao, "Adaptive tight frame based medical image reconstruction: a proof-of-concept study for computed tomography," *Inverse Prob.*, vol. 29, p. 125006, Dec. 2013.

[23] R. Zhang, D. H. Ye, D. Pal, J.-B. Thibault, K. D. Sauer, and C. A. Bouman, "A Gaussian mixture MRF for model-based iterative reconstruction with applications to low-dose X-ray CT," *IEEE Trans. Computational Imaging*, vol. 2, pp. 359–374, Sept. 2016.

[24] A. Aghasi and J. Romberg, "Sparse shape reconstruction," *SIAM J. Imaging Sci.*, vol. 6, no. 4, pp. 2075–2108, 2013.

[25] Q. Xu, H. Yu, X. Mou, L. Zhang, J. Hsieh, and G. Wang, "Low-dose X-ray CT reconstruction via dictionary learning," *IEEE Trans. Med. Imag.*, vol. 31, pp. 1682–1697, Sept. 2012.

[26] J. Liu, Y. Hu, J. Yang, Y. Chen, H. Shu, L. Luo, Q. Feng, Z. Gui, and G. Coatrieux, "3D feature constrained reconstruction for low dose CT imaging," *IEEE Trans. Circ. Sys. Vid. Tech.*, 2017. In Press.

[27] J. Luo, H. Eri, A. Can, S. Ramani, L. Fu, and B. De Man, "2.5D dictionary learning based computed tomography reconstruction," in *Proc. SPIE*, vol. 9847, pp. 98470L–1–98470L–12, 2016.

[28] R. Rubinstein, T. Peleg, and M. Elad, "Analysis K-SVD: A dictionary-learning algorithm for the analysis sparse model," *IEEE Trans. Sig. Proc.*, vol. 61, pp. 661–677, Feb. 2013.

[29] S. Ravishankar and Y. Bresler, "Learning sparsifying transforms," *IEEE Trans. Sig. Proc.*, vol. 61, pp. 1072–1086, Mar. 2013.

[30] S. Ravishankar and Y. Bresler, "ℓ_0 sparsifying transform learning with efficient optimal updates and convergence guarantees," *IEEE Trans. Sig. Proc.*, vol. 63, pp. 2389–2404, May 2015.

[31] S. Ravishankar and Y. Bresler, "Learning doubly sparse transforms for images," *IEEE Trans. Image Process.*, vol. 22, no. 12, pp. 4598–4612, 2013.

[32] B. Wen, S. Ravishankar, and Y. Bresler, "Video denoising by online 3d sparsifying transform learning," in *IEEE International Conference on Image Processing (ICIP)*, pp. 118–122, 2015.

[33] B. Wen, S. Ravishankar, and Y. Bresler, "Learning flipping and rotation invariant sparsifying transforms," in *IEEE International Conference on Image Processing (ICIP)*, pp. 3857–3861, 2016.

[34] S. Ravishankar and Y. Bresler, "Efficient blind compressed sensing using sparsifying transforms with convergence guarantees and application to magnetic resonance imaging," *SIAM Journal on Imaging Sciences*, vol. 8, no. 4, pp. 2519–2557, 2015.

[35] L. Pfister and Y. Bresler, "Model-based iterative tomographic reconstruction with adaptive sparsifying transforms," in *Proc. SPIE*, vol. 9020, pp. 90200H–1–90200H–11, 2014.

[36] L. Pfister and Y. Bresler, "Tomographic reconstruction with adaptive sparsifying transforms," in *Proc. IEEE Conf. Acoust. Speech Sig. Proc.*, pp. 6914–6918, 2014.

[37] L. Pfister and Y. Bresler, "Adaptive sparsifying transforms for iterative tomographic reconstruction," in *Proc. 3rd Intl. Mtg. on image formation in X-ray CT*, pp. 107–110, 2014.

[38] B. Wen, S. Ravishankar, and Y. Bresler, "Structured overcomplete sparsifying transform learning with convergence guarantees and applications," *Intl. J. Comp. Vision*, vol. 114, no. 2-3, pp. 137–167, 2015.

[39] J. A. Fessler and S. D. Booth, "Conjugate-gradient preconditioning methods for shift-variant PET image reconstruction," *IEEE Trans. Im. Proc.*, vol. 8, pp. 688–699, May 1999.

[40] H. Erdoğan and J. A. Fessler, "Ordered subsets algorithms for transmission tomography," *Phys. Med. Biol.*, vol. 44, pp. 2835–2851, Nov. 1999.

[41] Z. Yu, J.-B. Thibault, C. A. Bouman, K. D. Sauer, and J. Hsieh, "Fast model-based X-ray CT reconstruction using spatially non-homogeneous ICD optimization," *IEEE Trans. Im. Proc.*, vol. 20, pp. 161–175, Jan. 2011.

[42] S. Ramani and J. A. Fessler, "A splitting-based iterative algorithm for accelerated statistical X-ray CT reconstruction," *IEEE Trans. Med. Imag.*, vol. 31, pp. 677–688, Mar. 2012.

[43] D. Kim, S. Ramani, and J. A. Fessler, "Combining ordered subsets and momentum for accelerated X-ray CT image reconstruction," *IEEE Trans. Med. Imag.*, vol. 34, pp. 167–178, Jan. 2015.

[44] H. Nien and J. A. Fessler, "Relaxed linearized algorithms for faster X-ray CT image reconstruction," *IEEE Trans. Med. Imag.*, vol. 35, pp. 1090–1098, Apr. 2016.

[45] X. Zheng, Z. Lu, S. Ravishankar, Y. Long, and J. A. Fessier, "Low dose CT image reconstruction with learned sparsifying transform," in *Proc. IEEE Wkshp. on Image, Video, Multidim. Signal Proc.*, pp. 1–5, July 2016.

[46] I. Y. Chun, X. Zheng, Y. Long, and J. A. Fessler, "Efficient sparse-view X-ray CT reconstruction using ℓ_1 regularization with learned sparsifying transform," in *Proc. Intl. Mtg. on Fully 3D Image Recon. in Rad. and Nuc. Med*, 2017. Accepted.

[47] J. H. Cho and J. A. Fessler, "Regularization designs for uniform spatial resolution and noise properties in statistical image reconstruction for 3D X-ray CT," *IEEE Trans. Med. Imag.*, vol. 34, pp. 678–689, Feb. 2015.

[48] W. P. Segars, M. Mahesh, T. J. Beck, E. C. Frey, and B. M. W. Tsui, "Realistic CT simulation using the 4D XCAT phantom," *Med. Phys.*, vol. 35, pp. 3800–3808, Aug. 2008.

[49] Z. Wang, A. C. Bovik, H. R. Sheikh, and E. P. Simoncelli, "Image quality assessment: from error visibility to structural similarity," *IEEE Trans. Im. Proc.*, vol. 13, pp. 600–612, Apr. 2004.

[50] S. Ravishankar and Y. Bresler, "MR image reconstruction from highly undersampled k-space data by dictionary learning," *IEEE Trans. Med. Imag.*, vol. 30, pp. 1028–1041, May 2011.

[51] Y. Pati, R. Rezaiifar, and P. Krishnaprasad, "Orthogonal matching pursuit : recursive function approximation with applications to wavelet decomposition," in *Asilomar Conf. on Signals, Systems and Comput.*, pp. 40–44 vol.1, 1993.

[52] Q. Ding, Y. Long, X. Zhang, and J. A. Fessler, "Modeling mixed Poisson-Gaussian noise in statistical image reconstruction for X-ray CT," in *Proc. 4th Intl. Mtg. on image formation in X-ray CT*, pp. 399–402, 2016.

[53] S. Ravishankar, B. Wen, and Y. Bresler, "Online sparsifying transform learning – part I: Algorithms," *IEEE Journal of Selected Topics in Signal Processing*, vol. 9, no. 4, pp. 625–636, 2015.

[54] S. Ravishankar and Y. Bresler, "Online sparsifying transform learning – part II: Convergence analysis," *IEEE Journal of Selected Topics in Signal Processing*, vol. 9, no. 4, pp. 637–646, 2015.

PWLS-ULTRA: An Efficient Clustering and Learning-Based Approach for Low-Dose 3D CT Image Reconstruction: Supplementary Material

This supplement provides additional descriptions and experimental results to accompany our manuscript.

VII. Computing $\mathbf{D}_{\mathsf{R}}$ in Algorithm 1

Recall the following definition of $\mathbf{D}_{\mathsf{R}}$ in 11:

$$\mathbf{D}_{\mathsf{R}} \triangleq 2\beta \left\{ \max_k \lambda_{\max}(\mathbf{\Omega}_k^T \mathbf{\Omega}_k) \right\} \sum_{k=1}^{K} \sum_{j \in C_k} \tau_j \mathbf{P}_j^T \mathbf{P}_j. \quad (14)$$

When $\{\tau_j\}$ are all identical (or by replacing them with $\max_j \tau_j$ above for a looser majorizer), $\sum_{k=1}^{K} \sum_{j \in C_k} \mathbf{P}_j^T \mathbf{P}_j = \sum_{j=1}^{\tilde{N}} \mathbf{P}_j^T \mathbf{P}_j \in \mathbb{R}^{N_p \times N_p}$ is a diagonal matrix with the diagonal entries corresponding to image voxel locations and their values being the total number of image patches overlapping each voxel. Moreover, if the patches are periodically positioned with a stride of 1 voxel along each dimension and wrap around at image boundaries, then $\sum_{j=1}^{\tilde{N}} \mathbf{P}_j^T \mathbf{P}_j = l\mathbf{I}$. More generally, when τ_j values differ, we compute $\sum_{k=1}^{K} \sum_{j \in C_k} \tau_j \mathbf{P}_j^T \mathbf{P}_j$ voxel-wise by summing the τ_j values of the patches overlapping the voxel.

VIII. Additional Experimental Results

Section IV-D and Table II compared the performance of various methods for low-dose cone-beam (3D) CT reconstruction, for the XCAT phantom volume. Fig. 10 shows the reconstructions and the corresponding error (magnitudes) images (shown for the central axial, sagittal, and coronal planes) at $I_0 = 5 \times 10^3$ for FDK, PWLS-EP, PWLS-ST (with $\tau_j = 1 \ \forall \ j$), and PWLS-ULTRA ($K = 15$) with patch-based weights τ_j. PWLS-ULTRA provides better reconstructions and reconstruction errors compared to the conventional FDK and the non-adaptive PWLS-EP. PWLS-ULTRA also outperforms the proposed PWLS-ST scheme, and provides better reconstructions of image edges.

While Section IV-E and Fig. 8 showed the central axial plane of the chest volume reconstructed from low-dose helical CT data, Fig. 11 shows the PWLS-EP and PWLS-ULTRA ($K = 5$ and with patch-based weights τ_j) reconstructions for the central axial, sagittal, and coronal planes. For the sagittal and coronal planes, we show intensities from the central 135 of the 222 axial slices. The PWLS-ULTRA reconstruction clearly has reduced noise as well as higher resolution and better structural details and image edges than the PWLS-EP result.

Recall that in Section IV-E, we used the transforms learned from the patches of the XCAT phantom volume to perform reconstruction of the chest volume from low-dose helical CT data. Alternatively, one could learn the transforms from the patches of the PWLS-EP reconstruction of the helical CT data. Fig. 12 shows the square transforms ($K = 1$) learned from $8 \times 8 \times 8$ patches of the phantom and the PWLS-EP chest

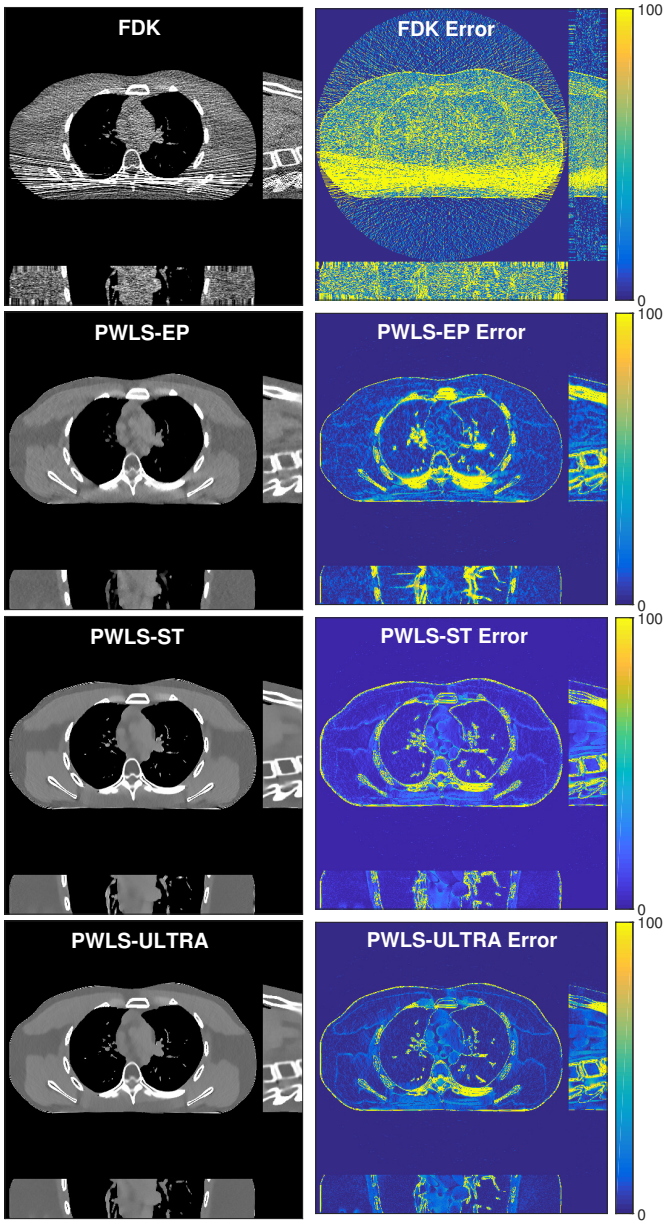

Fig. 10. Comparison of the reconstructions and corresponding error images (shown for the central axial, sagittal, and coronal planes) for FDK, PWLS-EP, PWLS-ST ($\tau_j = 1, \ \forall \ j$), and PWLS-ULTRA ($K = 15$) with patch-based weights τ_j at $I_0 = 5 \times 10^3$.

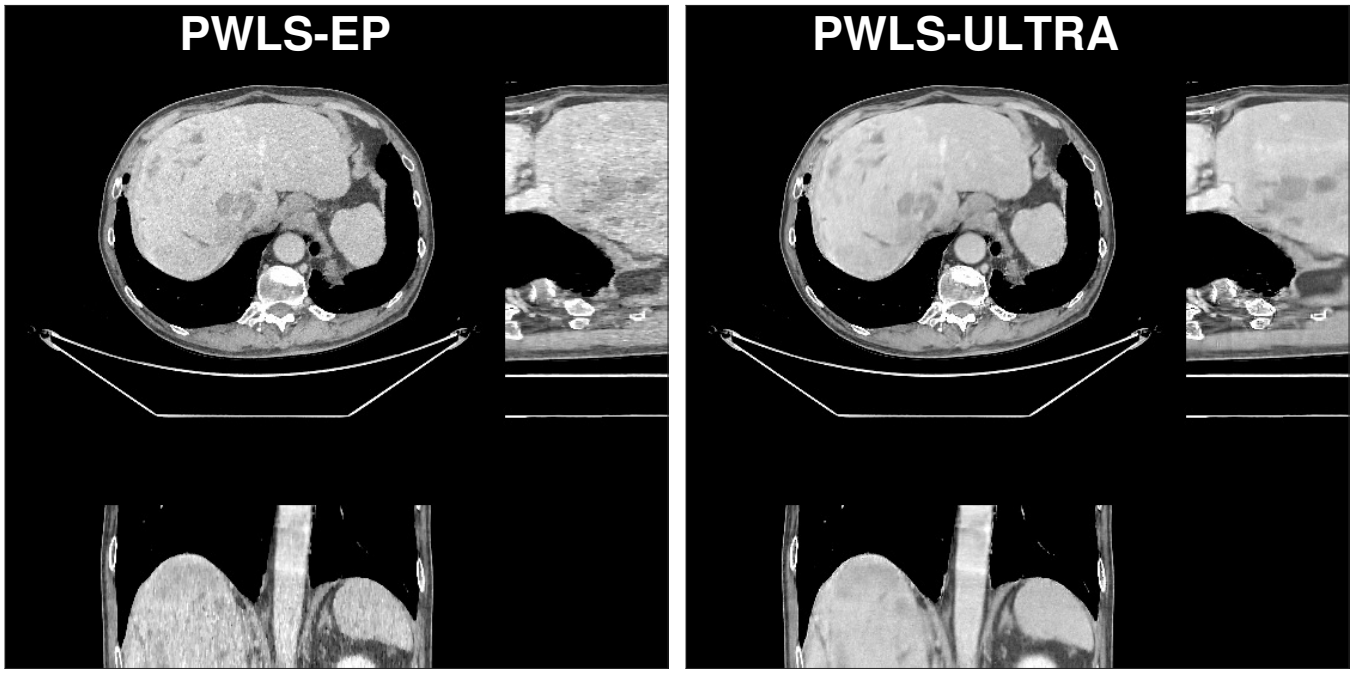

Fig. 11. Chest reconstructions (shown for the central axial, sagittal, and coronal planes) from low-dose helical CT data for the PWLS-EP and PWLS-ULTRA ($K = 5$) methods. For the sagittal and coronal planes, we show intensities from the central 135 of the 222 axial slices. The patch-based weights τ_j are used in PWLS-ULTRA.

reconstruction, with $\eta = 100$. These transforms display similar types of features, and provide similar visual reconstructions in PWLS-ST (with patch-based weights τ_j) in Fig. 12. Thus, the transform learning algorithm extracts quite general and effective sparsifying features for images, without requiring a very closely matched training dataset.

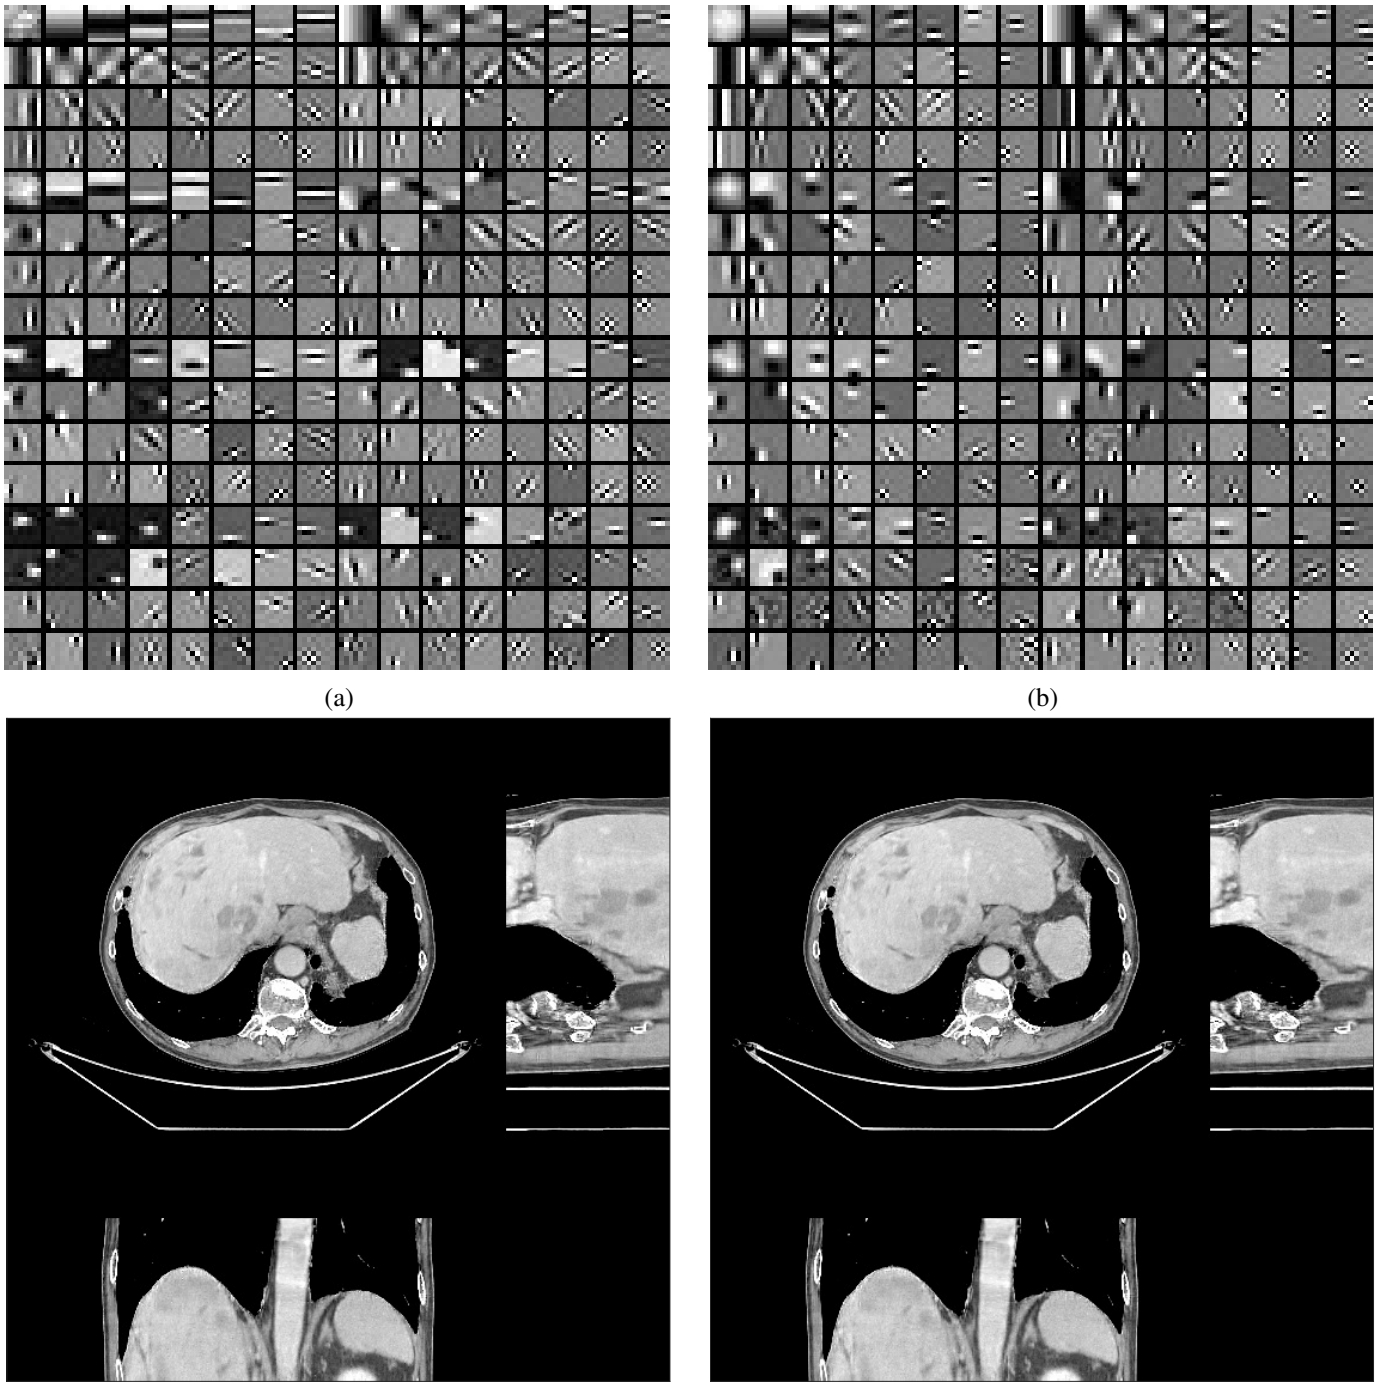

Fig. 12. The square transforms learned (with $\eta = 100$) from patches of the XCAT phantom and from patches of the PWLS-EP reconstruction of the helical CT data are shown in (a) and (b), respectively. Only the first 8×8 slice of 256 (among 320) $8 \times 8 \times 8$ atoms are displayed. (c) and (d) are the corresponding PWLS-ST reconstructions (shown for the central axial, sagittal, and coronal planes) obtained with the transforms in (a) and (b). For the sagittal and coronal planes, we show intensities from the central 135 of the 222 axial slices. We used the patch-based weights τ_j in PWLS-ST.